


ATWATER KENT MFG. CO.

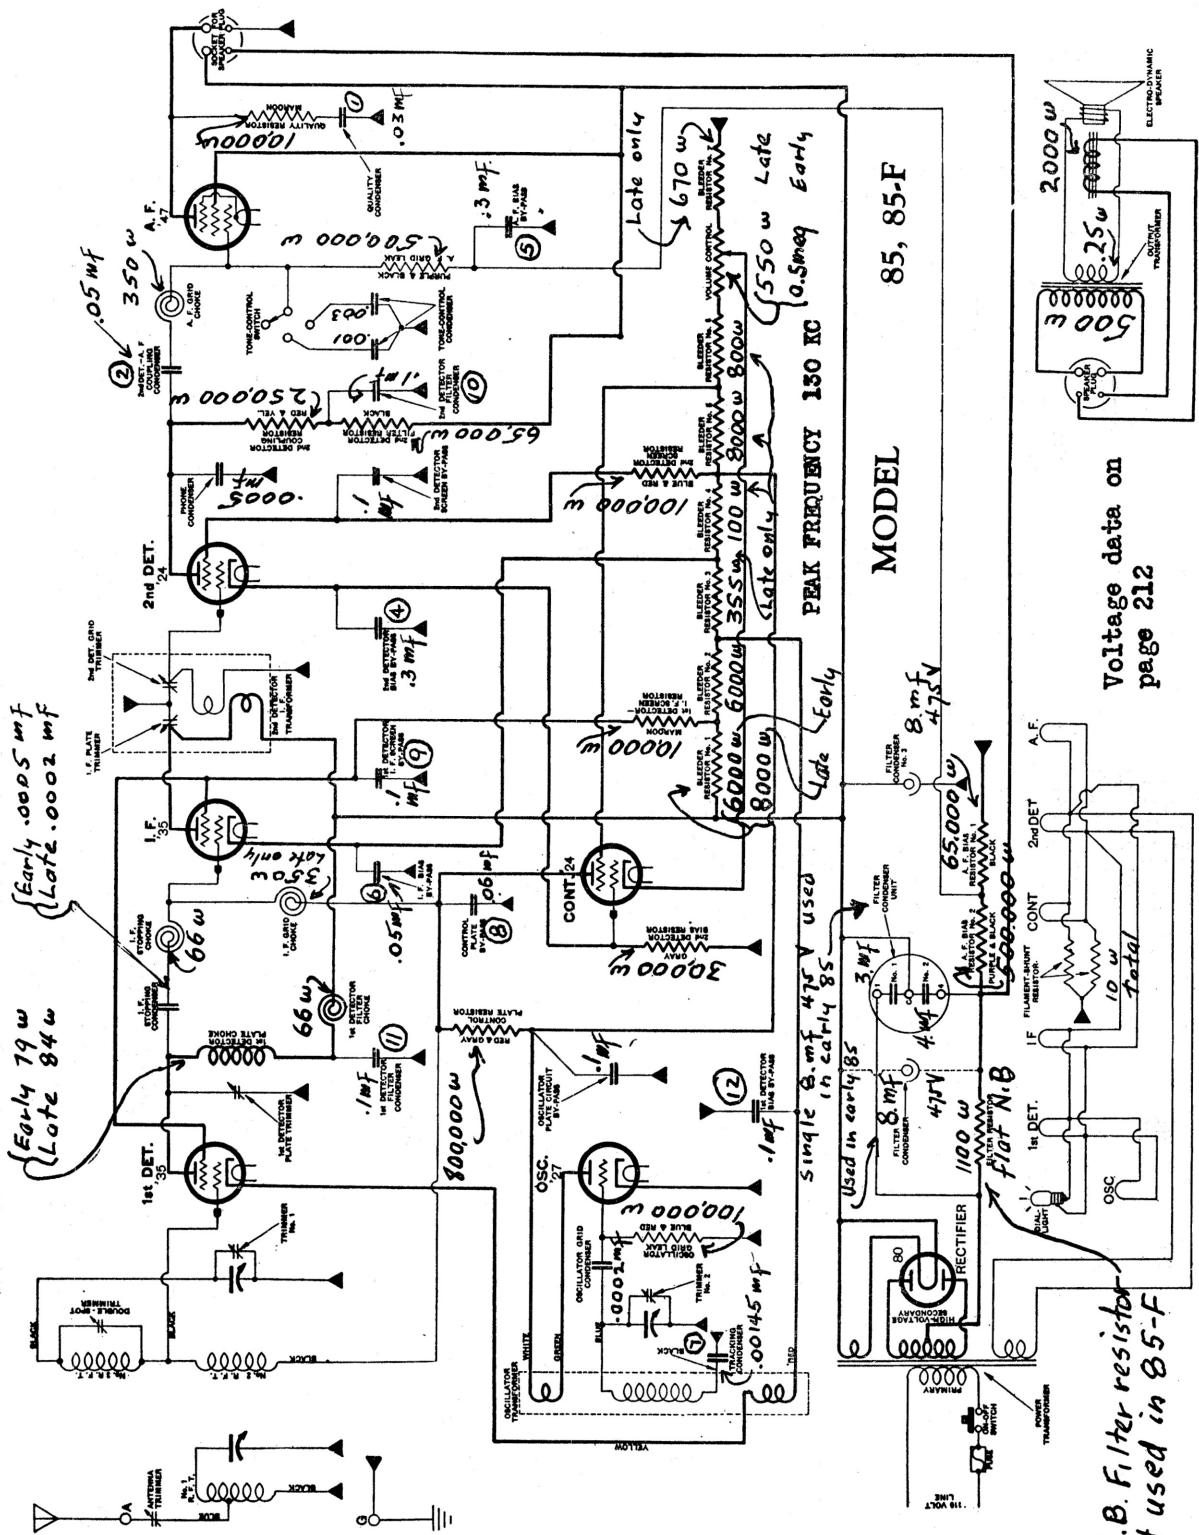

A few early-type Model 85 do not have automatic volume control; they have three electrolytic filter condensers; the circuit of these early Model 85 sets is similar to Model 80. The tracking condenser is mounted on the oscillator transformer in Model 82 and some 85 sets. The filament circuit of Model 82 is somewhat different from that shown above.